


**Robust . Reliable . Accurate**

# Handheld Miniature AOTF-NIR Analyzer



- Non-destructive Analytical Testing and Inspection
- Brimrose Analytical Software - Snap32!
- Multi-point, Multi-component Capability

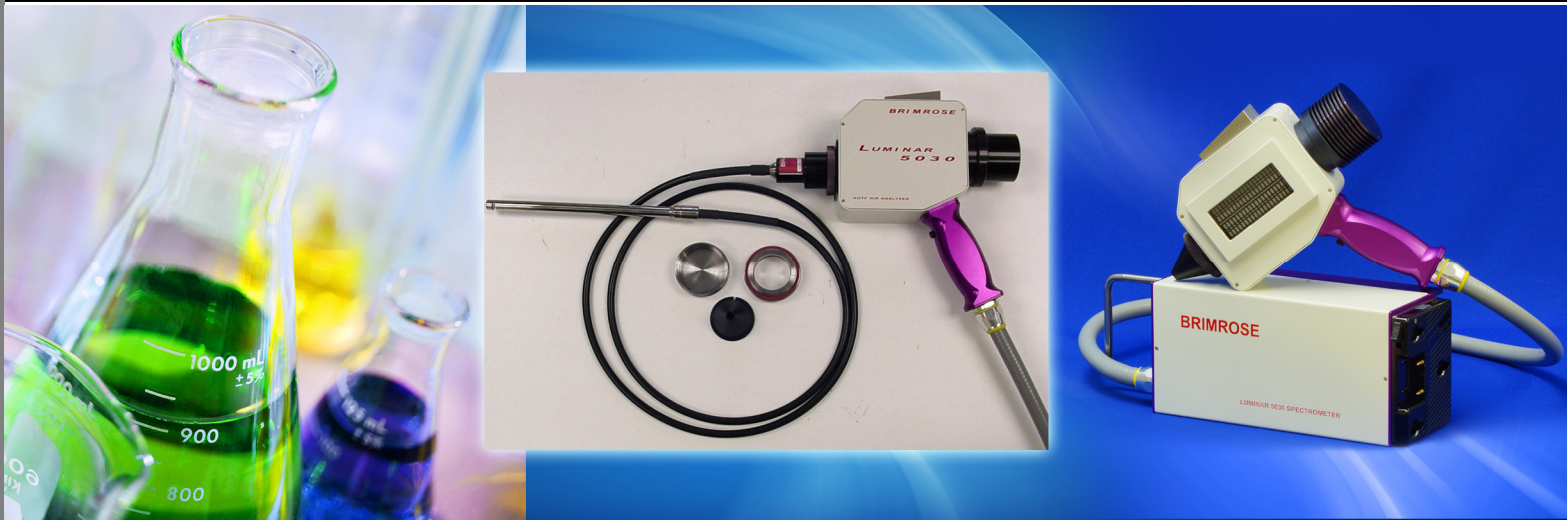

Brimrose Corporation of America  
Email: [office@brimrose.com](mailto:office@brimrose.com)  
[www.brimrose.com](http://www.brimrose.com)

Luminar 5030

## ■ Rugged Hand-held Analytical Instrument for Process Quality Control

Brimrose has developed a portable platform for conducting non-destructive and contact/non-contact analytical testing and inspection that extends versatility from the laboratory to the production floor and to the field.

The Brimrose Solid-state Luminar 5030 "Hand-held" Miniature AOTF-NIR (Acousto-Optic Tunable Filter-Near Infrared) Analyzer is a rugged hand-held analytical instrument that utilizes Brimrose's high performance AOTF-NIR technology. By delivering rapid, multi-component analysis for a wide variety of applications that include diffuse reflectance measurements of powders, pellets, liquids, web-based and solid products, use of the Luminar 5030 offers a new powerful tool for quality control and process troubleshooting. Additional probe attachments allow to use same analyzer for liquid transmission measurements.



**Diffuse Probe Attachment (optional)**

### ■ Measurement

- Moisture
- Fat/Sugar/Protein
- Active Ingredients
- Coating Weight
- Blend Assay
- Recycled Plastic ID



### ■ Key Features

- Dual Beam, Pre-aligned Lamp Assembly, InGaAs Detectors
- Fast Scanning Speed - 16,000 wavelengths/sec
- SNAP32! Brimrose Analytical Software with Brimrose MACRO Language
- 6mm Diameter Sample Area at 40mm Sampling Distance

### ■ Real-time Applications

- On-line Blend Uniformity
- FBD in Micro-encapsulation and Drying Process
- Incoming Raw Material Inspection
- Agricultural/Food: On-line food analysis for fat, protein, moisture, starch, etc.
- Polymer: Measurements of pellets and resins
- Paper and Textile Goods: On-Line thickness measurements
- Measurements of Tobacco and Tobacco Leaves
- Wine and Grape Applications: Measurements for Brix, pH, TA, etc.



**Brimrose Corporation of America**  
 Email: [office@brimrose.com](mailto:office@brimrose.com)  
[www.brimrose.com](http://www.brimrose.com)

## ■ Technical Data Specifications

| Spectrometer Name  | Luminar 5030 Handheld AOTF-NIR Analyzer   |
|--|---|
| <b>Spectral Range Options</b>  | 600-1100 nm, 850-1700 nm, 900-1800 nm, 1100-2300 nm   |
| <b>Measurement Modes</b>   | Diffuse Reflection, liquid transmission with probe attachment   |
| <b>Spectral Resolution</b>   | 2-10 nm   |
| <b>Wavelength Accuracy</b>   | ± 0.5 nm  |
| <b>Wavelength Repeatability</b>  | ± 0.01 nm   |
| <b>Wavelength Increment</b>  | Software Selectable 1-10 nm   |
| <b>Ambient Light Rejection</b>   | > 10 <sup>6</sup>   |
| <b>Vibration Immunity</b>  | Blenders, Agro field operations, e.g. vineyards   |
| <b>S/N at 70% Range</b>  | < 30µabs in reflectance and transmission, for <5 seconds integration time   |
| <b>Wavelength Access Time</b>  | < 66 µsec   |
| <b>Photometric Range</b>   | 3.5 AU  |
| <b>Linearity</b>   | Better than 0.15%   |
| <b>Signal Digitalization</b>   | 16-bit A/D (1 part in 65,536)   |
| <b>Sampling Speed</b>  | 16,000 wavelength/sec   |
| <b>Sampling Area</b>   | Ø6 mm   |
| <b>Sampling Distance</b>   | 40 mm   |
| <b>Diagnostic</b>  | 10 Built-in monitoring sensors  |
| <b>Power Requirements</b>  | 12VDC, (24VDC special order), 90Watts, 110VAC 60Hz, 220VAC 50Hz   |
| <b>Outputs</b>   | PC Interface via Ethernet connection  |
| <b>Software Package</b>  | Windows-based analytical software for data acquisition  |
| <b>Options:</b>  | <b>Accessories:</b>   |
| <ul style="list-style-type: none"> <li>➤ Battery Operation</li> <li>➤ Display</li> <li>➤ Liquid Probe Attachment</li> <li>➤ Powder Probe Attachment</li> <li>➤ Wireless Communication</li> <li>➤ Gravity Switch</li> </ul> | 5030O: L-shape mounting plate with 1.5" Sapphire Window Assembly for Quick dismounting of Optical module<br>5030E: Mounting Plate for Electronics module for quick dismounting of Electronics module<br>731-09: Liquid Transflectance measurements with selectable path lengths<br>731-10: Diffuse Reflectance measurement with Sapphire ball<br>731-S: Stand with Rotating cup |



Brimrose Corporation of America

Email: [office@brimrose.com](mailto:office@brimrose.com)

[www.brimrose.com](http://www.brimrose.com)

Luminar 5030